



OXYGEN CONCENTRATORS

DIRECT
SUPPLY®



Get the Industry's Top Performers

Direct Supply offers the industry's widest selection of oxygen equipment from brands you trust. Our product experts will help you choose the best units for your staff and residents.

Contact your account manager at **1-800-634-7328** today to learn more about Direct Supply's lineup of quality respiratory equipment.

**DIRECT
SUPPLY**
Attendant.

PHILIPS
RESPIRONICS

CAIRE

drive | **DeVilbiss**
HEALTHCARE

Choose from a vast selection to meet your needs

Oxygen concentrators provide respiratory users with increased mobility and flexibility for their active lifestyles. We carry a wide selection of the top models from portable to stationary to fit your community's requirements.

5L Oxygen Concentrators



10L Oxygen Concentrators



Portable Oxygen Concentrators



SAVE BIG WHEN YOU OWN YOUR OXYGEN CONCENTRATORS

You could save your community thousands of dollars every year when you purchase oxygen concentrators rather than opting for costly rental contracts. Many communities find the purchase pays for itself in the first year!




Calculate your potential savings today at **DirectSupply.com/Oxygen.**

You'll not only see your savings analysis, but videos on preventive maintenance and a huge selection of products to suit your residents' needs, including options from Invacare – an industry leader in respiratory products.



5-Year Cost Comparison: Renting vs. Owning

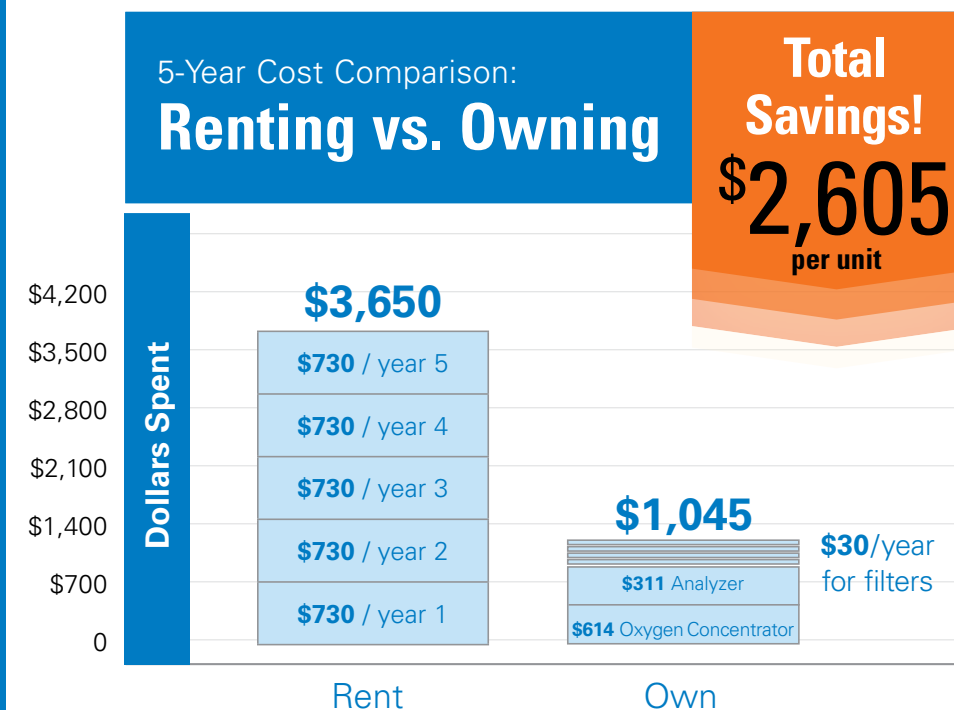

→ **EXAMPLE ONLY** – your savings may vary. Calculate your community's potential savings using our calculator.



Find more respiratory products on **DIRECTSUPPLY.NET**

5L Oxygen Concentrators

5L concentrators are a mobile and affordable way to provide up to 5 liters of continuous oxygen per minute to residents. Key selection criteria (in addition to price point) include sound level, required preventive maintenance steps and power consumption. Most brands offer optional built-in alarms for oxygen purity and flow rate, which can help provide peace of mind when owning concentrators. The comparison chart below provides a high-level overview of the models in our offering. Proceeding pages will provide additional detail on each model, including visual guides for preventive maintenance steps.



Attendant® 5L
Oxygen Concentrator

PAGE 6
#8X899



Caire® Companion 5™

PAGE 9
#C5319



Respironics EverFlo

PAGE 10
#96675,
#96676 (with O₂ Monitor)



DeVilbiss® Compact

PAGE 11
#17121

Manufacturer	Direct Supply	Caire
Unique Features	<ul style="list-style-type: none">Comes standard with oxygen purity and low flow rate indicatorsCompact footprint and lightweight design allows for easy storage and transportationTwo filters need attention only once a year under normal conditionsEasy-to-read digital hour meter display	<ul style="list-style-type: none">OPI oxygen monitor keeps track of purity levels; also available without monitorOnly two filters to change every 2 yearsReadout display provides an error code when alarms are onFlow meter ball drops to visually indicate loss of pressure for resident safety
Sound Level	≤50 dB	40 dB
Power Consumption	360W (average)	250W at 2 lpm, 350W at max
Warranty	3 years or 12,000 hours of compressor usage	Full 3 years with optional 2-year extention

Respironics	DeVilbiss
<ul style="list-style-type: none">OPI oxygen monitor keeps track of purity levels; also available without monitorOnly one filter to change every 2 yearsDurable metal cannula fittingRecessed flow meterUses capacitor rather than batteryFlow meter ball drops to visually indicate loss of pressure for resident safety	<ul style="list-style-type: none">Purity sensor attached to the concentrator checks the purity level of the oxygen, allowing caregivers to feel secure that the oxygen flowing is safe for the residentPressure-compensated flow meter displays accurate flowTurndown technology automatically activates at 2½ lpm or less to save energy and minimize stress on compressor
45 dB	48 dB
350W	310W at 5 liters per minute; 275W in Turn-Down (at or below 2½ lpm)
Full 3 years	Full 3 years

ATTENDANT® 5L OXYGEN CONCENTRATOR

5-LITER OXYGEN CONCENTRATOR



#8X899



- Trusted Attendant® brand
- Easy to maintain – just 2 filters are easily accessible and need attention annually
- Low flow rate and oxygen purity indicators standard
- Alarms for power failure, sensor failure and low flow lasting > 10 minutes

Specifications:	
Flow Rate:	0.5 - 5 lpm
O ₂ Purity %:	93%± 3%*
Outlet Pressure:	5 psi ± 6.23 psi
Power Consumption:	360W (average)
Sound Level:	≤50 db
Dimensions:	21 ³ / ₁₆ "H x 13"W x 10 ³ / ₁₆ "D
Weight:	36 lbs.
Warranty:	3 years or 12,000 hours of compressor usage

*0.5 - 5 LPM after running for 30 minutes

Preventive Maintenance

Once a Year:



Clean cabinet filter; replace intake filter

Once every 2 years:



Verify the oxygen purity, flow rate and pressure of your concentrator by using an oxygen analyzer.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.





CAIRE® COMPANION 5™

5-LITER OXYGEN CONCENTRATOR

Preventive Maintenance

Once Every 2 Years:



Check and, if necessary, change the air intake filter. We also recommend changing between residents.



Check and, if necessary, change the HEPA filter. Direct Supply suggests changing filter between residents.



Verify the oxygen purity, flow rate and pressure of your concentrator by using an oxygen analyzer.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.



#C5319

CAIRE®

- Maintains higher O₂ purity as flow rate increases
- Minimizes “exhale” noise for improved resident experience
- Reduces power consumption by 15% when running at 2 lpm or below
- Optional alarm screen displays error codes to specify technical issues
- Only two filters to change every 2 years – no weekly preventive maintenance

Specifications:	
Flow Rate:	0.5 - 5.0 lpm
O ₂ Purity %:	90% +5.5 / -3%
Outlet Pressure:	4.6 psi
Power Consumption:	250W at 2 lpm, 350W at max.
Sound Level:	40 dB
Dimensions:	12½"W x 13½"D x 21½"H
Weight:	36 lbs.
Warranty:	3 years*

RESPIRONICS EVERFLO

5-LITER OXYGEN CONCENTRATOR



#96676

PHILIPS
RESPIRONICS

- Recessed flow meter and metal output valve improve durability
- Optional alarms for oxygen purity and flow rate
- Only two filters to change every 2 years – no weekly preventive maintenance

Specifications:	
Flow Rate:	0.5 - 5.0 lpm
O ₂ Purity %:	90% - 96%
Outlet Pressure:	5½ psi
Power Consumption:	350W
Sound Level:	45 dB
Dimensions:	15"W x 9½"D x 23"H
Weight:	31 lbs.
Warranty:	3 years

*2-year extended warranty available

Preventive Maintenance

Once a Year:



Verify the power-loss alarm is working. Let the concentrator run for 1 minute then unplug the power cord. An alarm should sound, indicating it is working properly.

Once Every 2 Years:



Check and, if necessary, change the inlet compressor filter. We also recommend changing between residents.



Check and, if necessary, change the micro disc bacteria filter. We also recommend changing between residents.



Verify the oxygen purity, flow rate and pressure of your concentrator by using an oxygen analyzer.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.

Preventive Maintenance

Once a Week:



Clean the cabinet filter.

Once Every 2 Years:



Verify the power-loss alarm is working. Let the concentrator run for 1 minute then unplug the power cord. An alarm should sound, indicating it is working properly.



Inspect intake filter; replace as necessary.

Once Every 3 Years:



Check and, if necessary, change the final bacteria filter. We also recommend changing between residents.



Verify the oxygen purity, flow rate and pressure of your concentrator by using an oxygen analyzer.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.



#17121

drive | **DeVilbiss**
HEALTHCARE

- Purity sensor attached to the concentrator checks the purity level of the oxygen, allowing caregivers to feel secure that the oxygen flowing is safe for the resident
- Pressure-compensated flow meter displays accurate flow
- Turndown technology automatically activates at 2½ lpm or less to save energy and minimize stress on compressor

Specifications:	
Flow Rate:	1 to 5 lpm
O ₂ Purity %:	93% ±3% at all settings
Outlet Pressure:	8.5 psi
Power Consumption:	310W at 5 liters per minute; 275W in Turn-Down (at or below 2½ lpm)
Sound Level:	48 dB
Dimensions:	13½"W x 12"D x 24½"H
Weight:	36 lbs.
Warranty:	3 years

1-800-634-7328 • DirectSupply.net

10L Oxygen Concentrators



Drive DeVilbiss® Compact 10L
PAGE 13
#4HR15



Respironics Millennium M10
PAGE 14
#75875, #75876



AirSep® NewLife® Intensity 10
PAGE 15
#A9972 Single Flow, #A9974 Dual Flow

Manufacturer	Invacare	Respironics	AirSep
Unique Features	<ul style="list-style-type: none"> Assembled in the USA and compatible with cylinder transfill systems Lightweight with a small footprint Exclusive DeVilbiss OSD® (Oxygen Sensing Device), standard on every unit Equipped with accessible patient controls, bright LEDs, protected cannula fitting and recessed humidifier nook 	<ul style="list-style-type: none"> Optional O₂ percentage indicator ultrasonically measures O₂ output Durable casters for easy transport Large humidifier assembly area 	<ul style="list-style-type: none"> High outlet pressure designed to power high-acuity respiratory accessories: nebulizers, venti masks, long oxygen tubing Simplified tracheostomy setup with jet nebulizer attachment Several alarms for added security
Sound Level	55 dB	50 dB	55 dB
Power Consumption	639W	600W	590W
Outlet Pressure	20 +/- 1.0 psi	10 - 30 psi	20 psi
Warranty	3 years limited	Full 3 years with optional 2-year extention	Full 3 years with optional 2-year extention

10L concentrators provide up to 10 liters of oxygen per minute and are ideal for any residents with high flow needs, or those who are prescribed over 5 liters of oxygen per minute. Key selection criteria (in addition to price point) include sound level, preventive maintenance requirements, overall size, psi and presence of unique features. Higher psi levels are typically ideal for residents with longer tubing or trach connections. Some 10L models include unique features, such as dual flow meters and outputs, which allow up to 5 lpm of oxygen to be delivered to two different residents from one machine. Please review the information in the following pages to select the solution that best fits the needs of your residents.

DRIVE DEVILVISS® COMPACT 10L

10-LITER OXYGEN CONCENTRATOR



#4HR15

drive | DeVilbiss
HEALTHCARE

- Several audible and visual alarms: high pressure, high/low flow, low oxygen, power failure
- Oxygen Sensing Device (OSD) standard
- 3-year limited warranty

Specifications:	
Flow Rate:	2 - 10 lpm
O ₂ Purity %:	87% - 96%
O ₂ Pressure:	20 +/- 1.0 psi
Power Consumption:	639W
Sound Level:	55 dB
Dimensions:	13½"W x 12"D x 24½"H
Weight:	42 lbs.
Warranty:	3-year limited

Preventive Maintenance

Once a Week:



Clean the cabinet filter.

Once Every 2 Years:



Check and, if necessary, change the inlet compressor filter. We also recommend changing between residents.



Check and, if necessary, change the bacteria filter. We also recommend changing between residents or every 17,250 hours.



Verify the power-loss alarm is working. Let the concentrator run for 1 minute then unplug the power cord. An alarm should sound, indicating it is working properly.

Once Every 3 Years:



Verify the oxygen purity, flow rate and pressure of your concentrator by using an oxygen analyzer.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.

RESPIRONICS MILLENNIUM M10

10-LITER OXYGEN CONCENTRATOR



#75876

PHILIPS
RESPIRONICS

- Optional alarms for purity and flow rate
- Large humidifier bottle area
- Filters replaced every 2 years

Specifications:	
Flow Rate:	10 lpm (1-liter increments)
O ₂ Purity %:	92% ±4% at 8 - 10 lpm
	94% ±2% at 3 - 7 lpm
	92% ±4% at 1 - 2 lpm
O ₂ Pressure:	10 - 30 psi
Power Consumption:	600W
Sound Level:	less than 50 dB
Dimensions:	19"W x 13"D x 27"H
Weight:	53 lbs.
Warranty:	1 year

Preventive Maintenance

Once a Week:



Clean the cabinet filter.

Once Every 2 Years:



Check and, if necessary, change the inlet HEPA filter and pre-inlet filter. We also recommend changing between residents.



Check and, if necessary, change the bacteria filter. We also recommend changing between residents.



Check and, if necessary, change the long-life filter. We also recommend changing between residents.



Verify the oxygen purity, flow rate and pressure of your concentrator by using an oxygen analyzer.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.

AIRSEP® NEWLIFE® INTENSITY 10

10-LITER OXYGEN CONCENTRATOR



#A9974

AIRSEP®
A Chart Industries Company

- Available with single or dual flow meters and outputs
- Optional dual flow meter on 10 lpm models allows for two residents to receive up to 5 lpm at once
- Optional second output valve can be used for nebulizer treatments
- 20 psi output ideal for high flow needs

Preventive Maintenance

Once a Week:



Clean and, if necessary, change the intake (gross particle) filter. We also recommend changing between residents.

Once Every 5,000 Hours:



Check and, if necessary, change the felt filter. We also recommend changing between residents.

Once a Year:



Verify the power-loss alarm is working. Let the concentrator run for 1 minute then unplug the power cord. An alarm should sound, indicating it is working properly.

Once Every 2 Years:



Verify the oxygen purity, flow rate and pressure of your concentrator by using an oxygen analyzer.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.

Specifications:	
Flow Rate:	2 - 10 lpm
O ₂ Purity %:	92% at 2 - 9 lpm, 90% at 10 lpm
O ₂ Pressure:	20 psi
Power Consumption:	590W
Sound Level:	40 dB
Dimensions:	16½"W x 14½"D x 27½"H
Weight:	58 lbs.
Warranty:	3 years

Portable Oxygen Concentrators

Portable oxygen concentrators are the most lightweight and mobile O₂ delivery solutions available. Ranging from 4.4 to 20 lbs., these compact devices allow for AC, DC or battery power to allow oxygen therapy to be delivered while on the go. Resident activities, outside physician visits, general travel and power outages are popular reasons for using portable concentrators. Key selection criteria include flow rate (be sure to note differences between continuous and intermittent delivery options), battery life, size and weight. Please review the information on the following pages to select the solution that best fits the needs of your residents.



Respironics SimplyGo
PAGE 18
#A0065



Respironics SimplyGo Mini
PAGE 19
#E1773, #E1774



Caire® Eclipse 5®
PAGE 20
#C4575

Manufacturer	Respironics	Respironics	Caire
Flow Rate	0.5 - 2.0 continuous flow 1 - 6 lpm pulse in 0.5 lpm increments	0.5 - 3.0 lpm in 0.5 lpm increments	0.5 to 3.0 lpm continuous, 1 - 9 pulse settings
O ₂ Purity %	87% - 96%	90% +5.5 / -3%	90% +5.5 / -3%
Sound Level	≤43 dB at pulse setting 2	43dBA typical at pulse setting 2"	48 dBA at 3.0 lpm continuous flow; 40 dBA at 3.0 pulse dose setting
Battery Life	3½ hours / 7 hours with extra battery	4½ hours	2 hours at 2.0 lpm continuous flow
Dimensions	10"W x 6"D x 11½"H	8¾"W x 3¾"D x 9¾"H	12¾"W x 7¼"D x 19¾"H
Weight	10 lbs., 11.5 lbs. with extra battery	5 lbs.	18.4 lbs. with battery installed
Warranty	2 years	3-year on the system, 1-year on the sieve	3 years on concentrator, 1 year on battery and accessories



Caire® Freestyle® Comfort®
PAGE 21
#6YR11, #8VK42, #8VK43



Drive DeVilbiss® iGo2
PAGE 22
#347YR, #347YT



Drive DeVilbiss® iGo Ambulatory
PAGE 23
#7DJ14

Caire	Drive	Drive
1 - 5 pulse settings	1-5 pulse settings	1.0 - 3.0 lpm continuous flow, 1-6 pulse settings
90% +5.5 / -3%	90% +4/-3%	91% ±3%
40 dBA at pulse setting 2	37 dBA at pulse setting 2	40 dBA
Up to 4 hours with 8-cell battery pack. Up to 8 hours with 16-cell battery pack	3.5 hrs on pulse setting 2	1.6 to 4.0 hrs on continuous flow, 3.0 to 5.4 hrs on pulse settings 1-6
7¾"W x 3¼"D x 10"H	3.5"W x 8.6"D x 8.4"H	15" W x 11" D x 8" H
5 lbs.	4.95 lbs.	19 lbs. with battery
3 years on concentrator, 1 year on battery and accessories	5 years device, 3 years compressor, 1 year sieve beds and battery	3 years on concentrator, 1 year on battery

RESPIRONICS SIMPLYGO

PORTABLE OXYGEN CONCENTRATOR



#A0065



- Nonclinical style and ease of use make it appealing to residents
- Easy-to-remove battery for quick maintenance
- Multiple alarm types make troubleshooting easy

Specifications:	
Flow Rate:	0.5 - 2.0 continuous flow 1 - 6 lpm pulse in 0.5 lpm increments
O ₂ Purity %:	87% - 96%
O ₂ Pressure:	3 psi
Power Consumption:	150W while charging 120W while not charging
Sound Level:	≤ 43 dB at pulse setting 2
Battery Life:	3½ hours / 7 hours with extra battery
Dimensions:	10"W x 6"D x 11½"H
Weight:	10 lbs.; 11.5 lbs. with extra battery
Warranty:	2 years

Preventive Maintenance

Once Every 1 - 2 Years:



Check and, if necessary, change the inlet filter. We also recommend changing between residents.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.

RESPIRONICS SIMPLYGO MINI

PORTABLE OXYGEN CONCENTRATOR



#E1773 shown with brown backpack



Preventive Maintenance

Periodic intervals:



Clean and replace the cannula and tubing as instructed by the manufacturer and your equipment provider.

When changing residents:



Clean and disinfect the exterior covers of the device and rechargeable battery between patient use and as needed.

- Delivers the highest oxygen output for portable concentrators weighing 5 lbs or less
- External battery design is easy to install and change
- LCD touchscreen is easy to read and use
- Two battery option available: standard (up to 4.5 hrs) and extended (up to 9 hrs)

Specifications:	
Flow Rate:	0.5 - 3.0 lpm in 0.5 lpm increments
O ₂ Purity %:	90% +5.5/-3%
Sound Level:	43dBA typical at pulse setting 2"
Battery Life:	4½ hours
Dimensions:	83/10"W x 33/5"D x 92/5"H
Weight:	5 lbs.
Warranty:	3-year warranty on the system, 1-year warranty on the sieve

CAIRE® ECLIPSE 5®

PORTABLE OXYGEN CONCENTRATOR



#C4575



- Delivers the highest pulse dose oxygen output of any portable oxygen concentrator on the market
- Features autoSAT technology, which adjusts to the resident's respiratory rate as it increases and decreases
- Continuous flow settings 0.5 to 3.0 lpm (0.5 liter increments)

Specifications:	
Flow Rate:	0.5 - 3.0 lpm
Battery Life:	2 hours at 2 lpm continuous flow 5.1 hours at a 2 setting
O ₂ Purity %:	90% +5.5 / -3%
O ₂ Pressure:	5 psi
Power Consumption:	52W at 1.0 lpm continuous flow; 145W at 3.0 lpm; 45W at 1.0 pulse dose; 95W at 6.0 pulse dose
Sound Level:	45 dBA at 3.0 lpm continuous flow; 40 dBA at 3.0 pulse dose setting
Dimensions:	7 ¹ / ₁₀ "D x 12 ³ / ₁₀ "W x 19 ³ / ₁₀ "H
Weight:	15 lbs.
Warranty:	3 years

Preventive Maintenance

Daily:



Clean and, if necessary, change the air inlet filter or once per week. Replace annually.

Once a Year:



Replace the HEPA filter. We also recommend changing between residents.



Replace the compressor intake filter. We also recommend changing between residents.



Test the oxygen purity every time the device casing is opened, which is once annually as part of yearly preventive maintenance.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.

CAIRE® FREESTYLE® COMFORT®

PORTABLE OXYGEN CONCENTRATOR



#6YR11



- UltraSense sensitive breath technology
- Ergonomic shape
- Color display and glow in the dark keypad
- Long battery life up to 8 hours
- Internal filters designed to last the life of the device—no replacement needed

Preventive Maintenance

Once a Week:



Clean 2 air intake filters. Your oxygen provider may advise cleaning more frequently depending on operating conditions.

Every 3-6 months:



Replace the nasal cannula and tubing (every 3 months if daily use), or as recommended by the cannula manufacturer or you oxygen provider.

When changing residents:



Discard oxygen tubing, cannula/mask, oxygen outlet connector, and humidifier bottle. Replace cabin filter. Clean concentrator cabinet. Inspect plugs, cords and components. Check oxygen concentration.

Specifications:	
Flow Rate:	1 - 5 pulse settings
O ₂ Purity %:	90% +5.5/-3%
Sound Level:	40 dBA at pulse setting 2
Battery Life:	Up to 4 hours with 8-cell battery pack. Up to 8 hours with 16-cell battery pack
Dimensions:	7 ³ / ₁₀ "W x 3 ¹ / ₁₀ "D x 10"H
Weight:	5 lbs.
Warranty:	3 years on concentrator, 1 year on battery and accessories

DRIVE DEVILBISS® IGO2

PORTABLE OXYGEN CONCENTRATOR



#347YR,
#347YT

drive | DeVilbiss
HEALTHCARE

- SmartDose Auto-Adjusting Conserver Technology included
- Settings 1-5 pulse dose
- Rugged design, including protective overmold
- Weighs less than 5 lbs
- Most sensitive conserver trigger on the POC market

Specifications:	
Flow Rate:	1 - 5 pulse settings
O ₂ Purity %:	90% +4/-3%
Sound Level:	37 dBA at setting 2
Battery Life:	3.5 hours on pulse setting 2
Dimensions:	3.5"W x 8.6"D x 8.4"H
Weight:	4.95 lbs.
Warranty:	5 years device, 3 years compressor, 1 year sieve beds and battery

Preventive Maintenance

Periodic intervals:



Clean and replace the cannula and tubing as instructed by the manufacturer and your equipment provider.

When changing residents:



Clean and disinfect the exterior covers of the device and rechargeable battery between patient use and as needed.

DRIVE DEVILBISS® IGO AMBULATORY

PORTABLE OXYGEN CONCENTRATOR



#7DJ14

drive | DeVilbiss
HEALTHCARE

- Integrated PulseDose® oxygen conserving technology recognized for clinically effective pulse-dose oxygen delivery
- Built-in OSD® (oxygen sensing device) ensures accurate oxygen delivery and reduced periodic maintenance schedule
- Easy-to-read battery life gauge with fast battery charge time – 2 to 4.5 hours dependent upon the flow setting

Specifications:	
Flow Rate:	1.0 - 3.0 lpm continuous flow, 1-6 pulse settings
O ₂ Purity %:	91% ±3
Sound Level:	40 dBA
Battery Life:	1.6 to 4.0 hrs on continuous flow, 3.0 to 5.4 hrs on pulse settings 1-6
Dimensions:	15" W x 11" D x 8" H
Weight:	19 lbs with battery
Warranty:	3 years on concentrator, 1 year on battery

Preventive Maintenance

Weekly:



Clean Air Filter. Replace as needed and between patients.

Periodically:



Clean and replace the cannula and tubing as instructed by the manufacturer and your equipment provider

Every 3 Years:



Replace internal intake filter. We also recommend changing between residents.

When changing residents:



Clean and disinfect the exterior covers of the device and rechargeable battery between patient use and as needed.



1-800-634-7328 • DirectSupply.net